

Clinically Speaking

The Power of Seat Function and Base Selection

Power Mobility & Quantum Rehab



power
mobility
The power to move you


QUANTUM[®]
#1 FOR REHAB POWER

Agenda

- Assessment Process
- Mobility Equipment Algorithm
- Considerations for Power Wheelchair Prescription
- Advantages/Disadvantages of FWD, MWD and RWD
- Powered Seating
- Simple Programming

PEOP Model



Baum, C. M., Christiansen, C. H., & Bass, J. D. (2015). The Person-Environment-Occupation- Performance (PEOP) model. In C. H. Christiansen, C. M. Baum, & J. D. Bass (Eds.), *Occupational therapy: Performance, participation, and well-being* (4th ed., pp. 49-56). Thorofare, NJ: SLACK Incorporated.

Resource: Wheelchair Service Provision Guide

Wheelchair Service Provision

- Referral/Intake: Initial Interview
- Assessment/Initial Evaluation
- Equipment Recommendation/Selection
- Funding/Procurement
- Product Preparation (initial set up/programming)
- Fitting, Training, Delivery

Clinical Evaluation:

- Range of motion
- Strength
- Tone/spasticity
- Functional level
- Balance
- vision
- Cognition
- Plan of care and trajectory



<https://www.resna.org/Portals/0/Documents/Position%20Papers/RESNAWheelchairServiceProvisionGuide.pdf>

Assessment Process

power:
mobility
The power to move you



QUANTUM[®]

#1 FOR REHAB POWER

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Initial Assessment

Information Gathering
SCI Assessment form

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Medical History:

- **Primary Diagnosis**
- **Prognosis**
- **Medical History/Surgical History**
- Other Treatments or Rehab Measures trialed in the past
- Medications and allergies

Current Mobility Skills:

- **Safe, Timely, Independent**
- **Gait (Balance and Safety)**
- Manual Propulsion
- Power Mobility Control
- **Cardiopulmonary Tolerance (Vital Signs/Subjective Scales)**
- **Vision, Hearing, Cognition, Motor Control**

Neuromuscular:

- **Strength**
- Motor Control
- **Coordination**
- Tone/Spasticity
- Balance (sitting and standing)
- Vision and Hearing

Range of Motion and Flexibility

- **All body segments (including spine and pelvis)**
- Skeletal Deformity Assessment (Reducible vs Non-Reducible)
- **Linear Measurements**

Skin and Pain Assessment:

- **Current and Past Skin Integrity issues**
- **Risk Factors for Pressure Injuries**
- **Pressure Relief Ability**
- **Pain - when and where?**

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Goal Setting

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

If the need for a wheelchair is identified ask:

- Why?
- What is the purpose of the wheelchair?
- Where will it be used?
- How will this Mobility Device enable the participant to complete their task independently?
- SMART Goals

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Body ROM

NSW Health NSW State Spinal Cord Injury Service

Spinal Seating Professional Development Project

Assessment form part 2 (Basic MAT)

POSTURE IN CURRENT SEATING SYSTEM				
ASSESSMENT FOR:		DATE:		Problems /Comments
Pelvis	Tilt (Side view) <input type="checkbox"/> Neutral <input type="checkbox"/> Posterior <input type="checkbox"/> Anterior <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Obliquity (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Left Lower <input type="checkbox"/> Right Lower Lowered by: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Rotation (Top view) <input type="checkbox"/> Neutral <input type="checkbox"/> Left Forward <input type="checkbox"/> Right Forward <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	
Trunk	Anterior / posterior <input type="checkbox"/> Neutral <input type="checkbox"/> Thoracic Kyphosis <input type="checkbox"/> Lumbar Lordosis <input type="checkbox"/> Lumbar C-curve flattening <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Scoliosis (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Convex Left <input type="checkbox"/> Convex Right Apex at: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Rotation (Top view) <input type="checkbox"/> Neutral <input type="checkbox"/> L forward <input type="checkbox"/> R forward <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	
Hips	Thigh to Trunk angle: Left: _____ Degrees Right: _____ Degrees	Position (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Abduct* <input type="checkbox"/> Adduct* *L / R, *L / R <input type="checkbox"/> External rotation: L / R <input type="checkbox"/> Internal rotation: L / R	Windswept (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Left <input type="checkbox"/> Right	Left: Anoles Thigh - trunk: Thigh to lower leg: Lower leg to foot:
Knees and Feet	Thigh to lower leg angle: Left: _____ Degrees Right: _____ Degrees	Lower leg to foot angle: Left: _____ Degrees Right: _____ Degrees <input type="checkbox"/> Plantar-flex <input type="checkbox"/> Plantar-flex. <input type="checkbox"/> Dorsi-flex <input type="checkbox"/> Dorsi-flex.	Foot position: Left: <input type="checkbox"/> neutral <input type="checkbox"/> neutral <input type="checkbox"/> inversion <input type="checkbox"/> inversion <input type="checkbox"/> eversion <input type="checkbox"/> eversion	 Thigh - trunk: Thigh to lower leg: Lower leg to foot:
Head and neck	Cervical curve (side view) <input type="checkbox"/> Neutral <input type="checkbox"/> flexion <input type="checkbox"/> extension <input type="checkbox"/> cervical hyperextension (Chin poke)	Neck position (Frontal View) <input type="checkbox"/> Midline <input type="checkbox"/> Lat flexion: L / R <input type="checkbox"/> Rotation: L / R	Control <input type="checkbox"/> independent head control / and full ROM <input type="checkbox"/> restricted head control <input type="checkbox"/> restricted ROM: <input type="checkbox"/> absent head control	
Upper Limbs	Shoulder positioning <input type="checkbox"/> Level <input type="checkbox"/> asymmetry	Elbow and forearm position <input type="checkbox"/> arm support <input type="checkbox"/> no support	Wrist and handgrip	

SUPINE MAT ASSESSMENT																
ASSESSMENT FOR:		DATE:		Problems /Comments												
Pelvis	Tilt <input type="checkbox"/> Neutral <input type="checkbox"/> Posterior <input type="checkbox"/> Anterior <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Obliquity <input type="checkbox"/> Neutral <input type="checkbox"/> Left Lower <input type="checkbox"/> Right Lower Lowered by: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Rotation <input type="checkbox"/> Neutral <input type="checkbox"/> Left forward <input type="checkbox"/> Right forward <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Comments												
Trunk	Anterior / posterior <input type="checkbox"/> Neutral <input type="checkbox"/> Thoracic Kyphosis <input type="checkbox"/> Lumbar Lordosis <input type="checkbox"/> Lumbar C-curve flattening <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Scoliosis <input type="checkbox"/> Neutral <input type="checkbox"/> Convex Left <input type="checkbox"/> Convex Right Apex at: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Rotation <input type="checkbox"/> Neutral <input type="checkbox"/> Left forward <input type="checkbox"/> Right forward Forwarded by: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)													
Lower extremities	Angles Trunk to thigh angle: Flex hip to 90° or a lesser angle till ASIS mid / pelvic tilt Thigh to lower leg angle: with hip flex - at 90° or the trunk to thigh angle, extend knee from flexion till pelvic tilt / ASIS mid. Lower leg to foot angle:	Range of motions or report observations: <table border="1"> <tr> <th>LEFT</th> <th>RIGHT</th> <th>Normal ROM</th> </tr> <tr> <td></td> <td></td> <td>Simulate to 90°</td> </tr> <tr> <td></td> <td></td> <td>30 to 180</td> </tr> <tr> <td></td> <td></td> <td>30-135</td> </tr> </table>	LEFT	RIGHT	Normal ROM			Simulate to 90°			30 to 180			30-135	Foot / Heel: Connects with effort Note: Allow feet into trunk on resting position.	Left: Lower leg to foot: Thigh to lower leg: Thigh - trunk:
LEFT	RIGHT	Normal ROM														
		Simulate to 90°														
		30 to 180														
		30-135														
	Hip Abduction / Adduction:	Hip external / internal rotation:	Foot inversion / eversion:	Right: Lower leg to foot: Thigh to lower leg: Thigh - trunk:												
Head and neck	Cervical curve: Resting posture: <input type="checkbox"/> Neutral <input type="checkbox"/> Cervical Flexion <input type="checkbox"/> cervical hyperextension	Lateral flexion: Resting posture: <input type="checkbox"/> Neutral <input type="checkbox"/> left <input type="checkbox"/> right <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort	Rotation: Resting posture: <input type="checkbox"/> Neutral <input type="checkbox"/> left <input type="checkbox"/> right <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort													
Upper extremities	Shoulder PROM <input type="checkbox"/> Level <input type="checkbox"/> asymmetry	Elbow and forearm PROM	Wrist and hand Description:													


SITTING MAT ASSESSMENT					
ASSESSMENT FOR:		DATE:		Problems /Comments	
Pelvis	Balance: <input type="checkbox"/> Hands-free sitter <input type="checkbox"/> Hands dependant sitter <input type="checkbox"/> "Propped sitter" (* for advance still clinician / specialist only)	Tilt (Side view) <input type="checkbox"/> Neutral <input type="checkbox"/> Posterior <input type="checkbox"/> Anterior	Obliquity (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Left Lower <input type="checkbox"/> Right Lower Lowered by:	Rotation (Top view) <input type="checkbox"/> Neutral <input type="checkbox"/> Left forward <input type="checkbox"/> Right forward	Simulation & Outcome: (Describe direction and location of forces applied) Accommodations / corrections: Outcomes:
Trunk	Anterior / posterior <input type="checkbox"/> Neutral <input type="checkbox"/> Thoracic Kyphosis <input type="checkbox"/> Lumbar Lordosis <input type="checkbox"/> Lumbar C-curve flattening <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Scoliosis (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Convex Left <input type="checkbox"/> Convex Right Apex at: <input type="checkbox"/> fixed <input type="checkbox"/> flexible <input type="checkbox"/> corrects with effort (to neutral / partial correction)	Rotation (Top view) <input type="checkbox"/> Neutral <input type="checkbox"/> L forward <input type="checkbox"/> R forward		Accommodations / corrections: Outcomes:
Lower extremities	Initial sitting angles Thigh - trunk: Thigh to lower leg: Lower leg to foot:	Position (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Abduct* <input type="checkbox"/> Adduct* *L / R, *L / R <input type="checkbox"/> External rotation: L / R <input type="checkbox"/> Internal rotation: L / R	Windswept (Frontal View) <input type="checkbox"/> Neutral <input type="checkbox"/> Left <input type="checkbox"/> Right	Stimulated sitting angles: Thigh - trunk: Thigh to lower leg: Lower leg to foot:	
Head and neck	Cervical curve (side view)	Neck position (Frontal View)	Control	Accommodations / corrections: Outcomes:	
Upper Extremities	Shoulder positioning <input type="checkbox"/> Level <input type="checkbox"/> asymmetry Describe:	Elbow and forearm position Describe:	Hand and wrist positioning Describe:	Accommodations / corrections: Outcomes:	

https://aci.health.nsw.gov.au/_data/assets/pdf_file/0018/156060/m03_mat_basic.pdf

Linear Measurements

Does the AT equipment requested for trial meet the clients goals and objectives as stated in their plan? YES NO
It is preferable to have this information prior to booking a trial.

- A: Seat Width
- B: Seat Depth
- C: Lower Leg Length
- D: Seat Back Height
- E: Armrest Height
- F: Backrest Width
- Client Height
- Client Weight

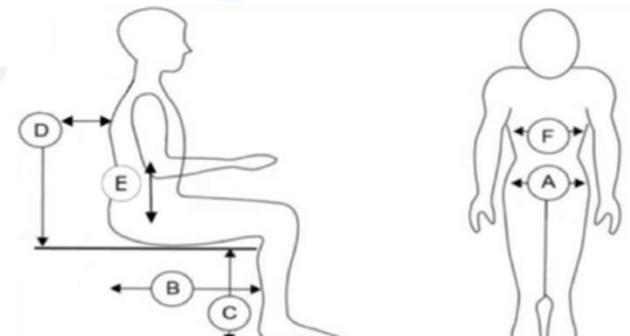

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Environmental Considerations

- Access in and around home
- Obstacles
- Type of terrain
- Inclines
- **Transportation**
- Access and manoeuvrability

Assessment Process

Initial Assessment / Information Gathering

Development of Goals

Physical Assessment / MAT Evaluation

Environmental Assessment

Equipment Trial Process

Clinical Reasoning

Equipment Considerations and Report Writing

Delivery and On-Going Training

Wheelchair Trial Process & Clinical Reasoning

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Mobility Assistive Equipment (MAE) - Algorithmic Process.

What MAE device allows the individual to go from Point A to Point B in an:

- *Independently*
- *Safely*
- *AND timely*

manner in order to accomplish MRADL's?

Gait Device



Manual Wheelchair



Scooter



Basic Power Wheelchair



Complex Power Wheelchair



Considerations:

- Cognition
- Upper Limb Function
- Vision
- Carer requirements
- Travel
- Changing/progressing condition

Power Seat Bases

Drive Wheel Configuration

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Drive Wheel Configurations



Rear Wheel Drive



Mid Wheel Drive



Front Wheel
Drive




4 Wheel
Drive



Drive Wheel Location

- ⊙ Geometric Centre
- ⊙ Centre of Head
- ★ Centre of Gravity
- ® Centre of Rotation

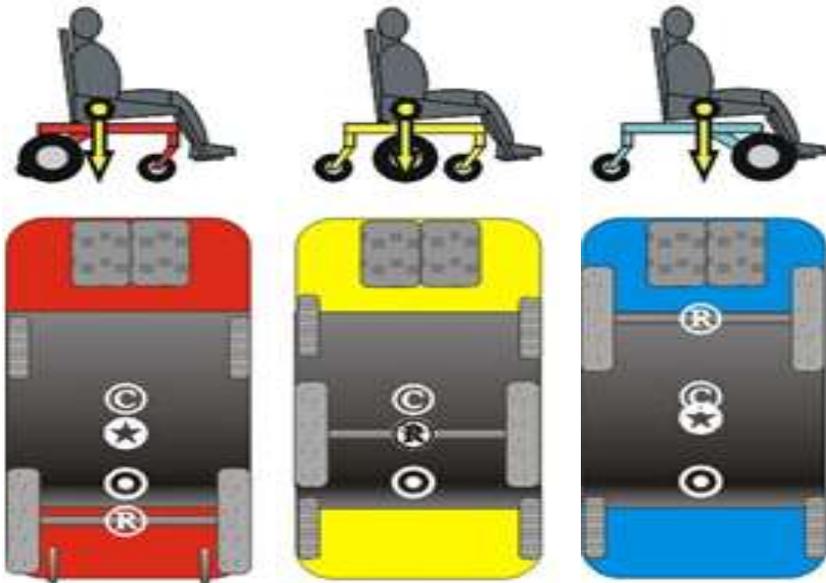

A Chair turns on the "**Center Point**" of the drive wheel axis

The closer the user's head is to the w/c center of rotation, the less rotational displacement

4FRONT²

Maximum speed –	10km/h 5.6km/h
Overall base size –	101.3cm Length 61.4cm Width
Seating -	12"-22" Wide 12"-22" Deep
Weight Capacity –	136kg



4FRONT² HD

Maximum speed –	10km/h 5.6km/h
Overall base size –	101.8cm Length 61.4cm Width
Seating -	20"-24" Wide 20"-24" Deep
Weight Capacity –	204kg



Front Wheel Drive – Advantages



- More force distributed to each of the **four tires**, because there are two fewer tires in contact with the ground
- Performs well when driving over a **range of terrains** – grass or uneven gravel.
- **Climbs well over obstacles.** The larger tires at the front “grab” an obstacle like a curb or a step and go over it, pulling the rest of the chair with it
- Accommodates for **tight hamstrings or compromised leg rest** positioning easily because there are no front caster wheels to interfere
- Easily navigate **tight corners** within the home
- **Front Access** to work surfaces

Front Wheel Drive – Disadvantages



- Anti-tip casters can interfere with foot placement for stand pivot transfers
- Turning in tight spaces can be tricky for new users because more of the chair is behind them
- Harder to drive straight at higher speeds -Directional Stability decreases as the speed of chair increases (Fishtailing)
- May have less control with non-proportional drive input device
- Not a great base for attendant only use



QUANTUM[®] EDGE[®] 4

Maximum speed –	10km/h 7.1km/h with iLevel
Turning radius –	57.9cm
Overall base size –	82cm Length 62.2cm Width
Seating -	12"-22" Wide 12"-22" Deep
Battery Size –	70amp
Cator Size -	7"
Weight Capacity –	150kg



FDA Class II Medical Device



EDGE 3 *Stretto*



- Maximum speed –** 10km/h
5.6km/h with iLevel
- Turning radius –** 53.3cm
- Overall base size –** 82.5cm Length
52cm Width
- Seating -** 12"-20" Wide
12"-20" Deep
- Range Per Charge –** Up to 25km
- Weight Capacity –** 136kg



Q6 edge[®] HD



Maximum speed –	7.6km/h
Turning radius –	54cm
Overall base size –	90.4cm Length 66.68cm Width
Seating -	20"-28" Wide 20"-25" Deep
Range Per Charge –	Up to 25km
Weight Capacity –	204kg



Mid Wheel Drive – Advantages



- Tightest turning radius for a 360° turn
- Most **intuitive** to drive as the COG is closest to the chair's center point
- **Climbs obstacles fairly well** - can be limited by how high caster wheels lift
- Having 6 wheels on the ground provides **stability** to the base
- **Good traction** on most surfaces, inclines and side slopes
- **Versatile** – Great for indoors and outdoors

Mid Wheel Drive – Disadvantages



- Can high center on very uneven terrains – challenge for gutters
- Have limitations in the height of obstacle they can climb with smaller front castors
- Front caster wheels can interfere with stand pivot transfers
- Front caster wheels can be problematic for individuals with tight hamstrings or longer lower leg lengths



R-TRAK



- Maximum speed –** 10km/h
5.6km/h
- Turning radius –** 65.8cm
- Overall base size –** 88.3cm Length
60cm Width
- Seating -** 12"-22" Wide
12"-22" Deep
- Range Per Charge –** Up to 25km
- Weight Capacity –** 136kg



Rear Wheel Drive – Advantages



- Provides good control at higher speeds
- Handles aggressive terrain very well
- Large Front Castors = Smoother Ride Outdoors
- May be familiar for some users
- Most intuitive for attendants to use



Rear Wheel Drive – Disadvantages



- May have access issues due to large turning radius
- Front caster wheels can interfere with footplate placement
- Front caster wheels can be problematic for individuals with tight hamstrings
- More likely to tip backwards when going up hill, as batteries and motor are at the rear of the chair



QUANTUM®
OUTBACK

MAKE YOUR OWN PATH



- Drive wheels –** 14” pneumatic tires
- Ground Clearance –** 10.7cm
- Drivetrain –** 4 motor, independent drive
- Battery Size –** (2) 95AH
- Weight Capacity –** 160kg



Off Road – Advantages

- Large pneumatic tires combined with suspension provide smooth ride
- Independent motors on each wheel
- Handles off road terrain well
 - Sand
 - Kerbs/ rocks
 - Farmland



Off Road – Disadvantages

- Large turning circle
- Hard to reverse
- Bulkiness and transportability
 - Indoor access
- Not designed for attendant control
- Maintenance
- Transfers




Case Study – Cam

- C7 incomplete quad
- Everyday chair – Push chair manual indoor chair, Quantum Edge 3 PWC
- Barrier – Cam’s current wheelchairs are not able to access rough or loose surface terrains.
- Goals – Cam would like to access the beach and local hiking trails with his friends.



Case Study – Cam



Maintenance and support

- Regular Servicing is Essential – Prevents breakdowns & extends chair lifespan
- User Responsibility – Basic care & daily checks
 - Tyre Care
 - Batteries
 - Saltwater care

Is There a Drive Wheel Configuration that is “Best” for an Individual’s Life Style?



Activity

- Split into groups & focus on tight turning and using the attendant controls -
 - Mid Wheel Drive
 - Front Wheel Drive
 - Rear Wheel Drive
 - Off Road
- Which one felt the most natural?
- Which one was the hardest to control?

BREAK TIME!



power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Power Seat Functions

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Power Seat Functions



Anterior Tilt



Elevating Legs



Posterior Tilt



Elevate / Lift



Recline



Stand

Why PWC Users Change Position:



Pressure Relief



Improved Head /
Trunk Control



Balance & Stability



Functional Reach



Safe Negotiation of
Obstacles / Inclines

Posterior Tilt

Seat tilts posteriorly in relation to the ground, while maintaining the seat-to-back, and lower leg angle.



Benefits of Power Tilt

- **Pressure Relief**

- The more Tilt that is available, the better!
- >30° Defines a pressure relieving tilt
- 15° or less No advantage for pressure relief
- Up to 65° Significant ischial pressure relief
(www.resna.org)
- Recommendation is to maintain an offloaded position from the seating surface for at least 1 to 2 minutes every 30 minutes. (*Pressure Ulcer Prevention and Treatment Following Spinal Cord Injury: A Clinical Practice Guideline for Health-Care Professionals SECOND EDITION SPINAL CORD MEDICINE*, n.d.-a)

- **Positioning**

- Support users to maintain an optimal seated posture by minimizing effects of gravity.
- Improves stability while reducing energy output (driving, fatigue)
- Reduces sliding
- Independent repositioning

Pressure Ulcer Prevention and Treatment Following Spinal Cord Injury: A Clinical Practice Guideline for Health-Care Professionals SECOND EDITION SPINAL CORD MEDICINE. (n.d.-a).



Benefits of Power Tilt

Community Access and Stability

- Utilising tilt while accessing slopes or uneven terrain can support postural stability.
- Reduce risk of sliding forward when travelling down hills.
- Increase clearance under footplates when travelling up-hills or slopes.

Fatigue Management

- Increased sitting tolerance
- Energy conservation



Recline

Increases the seat to back angle, while maintaining the seat angle in relation to the ground.



Recline

Pressure Relief

- “The greatest reduction in pressures were seen when combinations of tilt and recline were used together, with studies using 25-45° of tilt with 110-150° of recline.” (RESNA Position on the Application of tilt, Recline, and Elevating Legrests for Wheelchairs: 2015 Current state of the Literatures)

Independent Repositioning

- Comfort - Increases sitting tolerance
- Passive Range Of Motion at hips
- May help to achieve a supine position

Balance and Stability

- Improve trunk stability
- Improves postural readiness



Recline

Reduces Manual Handling

Reduction of transfers required throughout the day
Reduces the need for transfers

Considerations:

Increased risk of shear

➤Tilt before recline decreases risk

Increased risk of Posterior Tilt/Sliding

Increased Risk of shifting access to drive controls and postural supports

Power Tilt and Recline

Clinical Benefits

- 25°- 45° Tilt with 110°- 150° Recline provides the **greatest pressure relief** when used in combination
- 45° of tilt with 120° of recline provides a **40% load reduction**
- Tilt before recline **decreases shear**
- Multiple angles provide ease of independent, or caregiver assisted repositioning
- 30° of tilt with full recline improves lower limb hemodynamic states (**edema**)
- Dynamic seating allows a variety of postures throughout the day to participate in or perform **ADLs**



Power Elevating Legs

Elevates leg supports to allow users to change the lower leg angle in relation to the seat and extend knees.



Benefits of Power Elevating Legrests

- Lower Edema Management
- Optimal pressure distribution
 - When used in conjunction with tilt and/or recline
- Positioning
 - Use with recline to aid in maintenance of pelvic position (prevention of posterior or anterior pelvic tilt)
 - Allow extension of knee
 - Independent repositioning
 - Centre-mount Vs Swing-Away supports
- Pain management
- Environmental access
 - Increase clearance under footplates where tilt is not appropriate
 - Achieve a reduced footprint for navigating tight spaces
 - Ability to get closer to benches/tables etc.



Considerations:

- Hamstring range
 - May result in sliding if not used in conjunction with backrest recline.

Seat Elevation / Lift

Allows the entire seating system to raise while maintaining angles.



Benefits of Seat Elevation

It is RESNA's position that power seat elevation devices are medically necessary,

as this technology enables certain individuals to:

- Facilitate reach biomechanics, safety and range
- Improve transfer biomechanics, safety and independence
- Enhance visual orientation and line-of-sight
- Support physiological health, safety and well-being
 - Decrease hyperlordotic position of the neck
 - Promote stable seated positioning
 - Improve safety with performance/participation in ADLs
- Promote communication, social engagement, self-esteem and integration
- Improve wheelchair pedestrian safety



RESNA Position of the Application of Seat Elevation Devices for Power Wheelchair Users: Update 2019
Current state of the Literatures

Case Study - Video



Anterior Tilt

Anterior tilt shifts the entire seating system forward by raising the rear seat to floor height while maintaining front seat to floor height.



What is Anterior Tilt?

- A power seating function that much like traditional posterior tilt changes the angle of the wheelchair seat in the sagittal plane.
- This function raises the posterior aspect of the seat higher than the front which places the person in a partial standing position.





Q

QUANTUM

#1 FOR REHAB POWER

TRU
BALANCE 4

POWER POSITIONING SYSTEM

30°
20°
10°
0°

TB4 Anterior Tilt Packages



0° - 10° Package



0° - 30° Package



What Bases come with TB4?

4FRONT²



STFH: 45 cm – 47.62 cm
Seat: 40.64 cm-55.88 cm W x
38.1 cm-55.88 cm D
Lift: 25.4 cm at 5.6 KPH
41.2 cm maximum lower leg
support recommendation
(measured from seat pan to
footplate)

All models:

Posterior tilt: 0-50°

Power Recline: 0-164°

New Dual Actuator AFP with power articulation to the floor

EDGE 3 *Stretto*



STFH: 45.72 cm-48.26 cm
Seat: 40.6 cm-55.88 cm W x
35.56 cm-55.88 cm D
Lift: 30.4 cm at 5.6 KPH
w/iLevel
39.3 cm maximum lower leg
support recommendation
(measured from seat pan to
footplate)

EDGE 3



STFH: 44.45 cm – 48.89 cm
Seat: 38.1 cm-55.88 cm W x
35.56 cm-55.88 cm D
Lift: 30.4 cm at 7.2 KPH w/iLevel
42.5 cm maximum lower leg
support recommendation
(measured from seat pan to
footplate)

What is required for TB4 Anterior Tilt?

- **All Power Actuators**

- Power Tilt
- Power Seat Elevation
- Power Recline
- Power LE Elevation
- Foot Platform Articulation



Clinical Benefits of Anterior Tilt

Position Change


Increase Functional Reach

Transfer Assistance

Visual Field Improvements

1) Position Change

- **Pain management**
- **Pressure re-distribution**
 - Additional functional movement options (dynamic seating) could increase the frequency in which weight shifts are completed
- **Increased activity tolerance**
 - Due to changes in joint angles and increased comfort/tolerance
- **Tone/spasticity management**
 - Joint angle changes

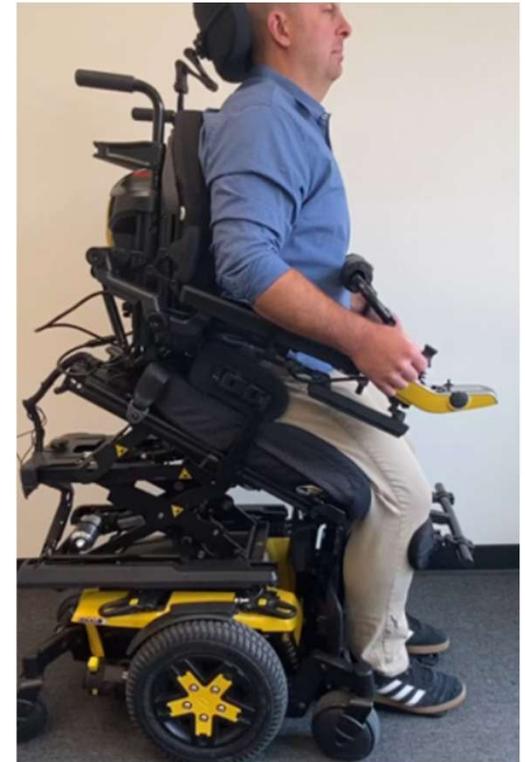

2) Increase Functional Reach


- **Increasing horizontal and vertical reach**
 - Improved upper extremity function even at anterior slopes of 0-15 degrees (Stavness, 2006).
- **Improved biomechanics for reaching**
- **Limit positions that cause impingement**
 - Limits internal rotation with abduction
- **Improve energy conservation**
 - “Wheelchair users perform overhead arm activities 5 times more often than ambulatory control subjects



Sharon E. Sonenblum , Chris L. Maurer , Christopher D. Hanes , Julie Piriano & Stephen H. Sprigle (2021)

Position Change For Balance and Reach:

- In many individuals reaching outside one's base of support may be limited
 - Extensive research on this for those with SCI, MS, post stroke, and CP

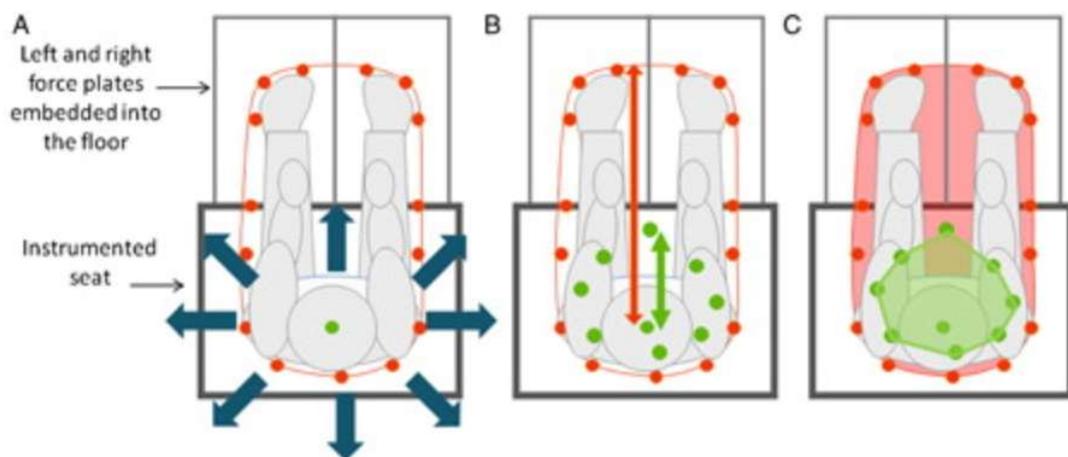

B. Red line is the maximal potential for center of pressure shift
-Green is the actual center of pressure achieved

C. green = average area of excursion possible

So, let's bring the person closer to their desired object to maximize this when it comes to reach and balance!

Case Study – Keli



Activities of Daily Living – Functional Tasks:

- Access to sinks
- Grooming
- Meal prep
- Reaching items in cupboards
- Accessing cooktop
- Doing laundry




Seat Elevation with Anterior Tilt is what allows the most OPTIMAL access

3) Transfer Assistance

- Improving independence during transfers
- Decreased caregiver burden for transfers
- Less strain on upper extremities
- Energy conservation
 - Preservation of lower extremity available strength and endurance if appropriate



Analysis of the Sit to Stand

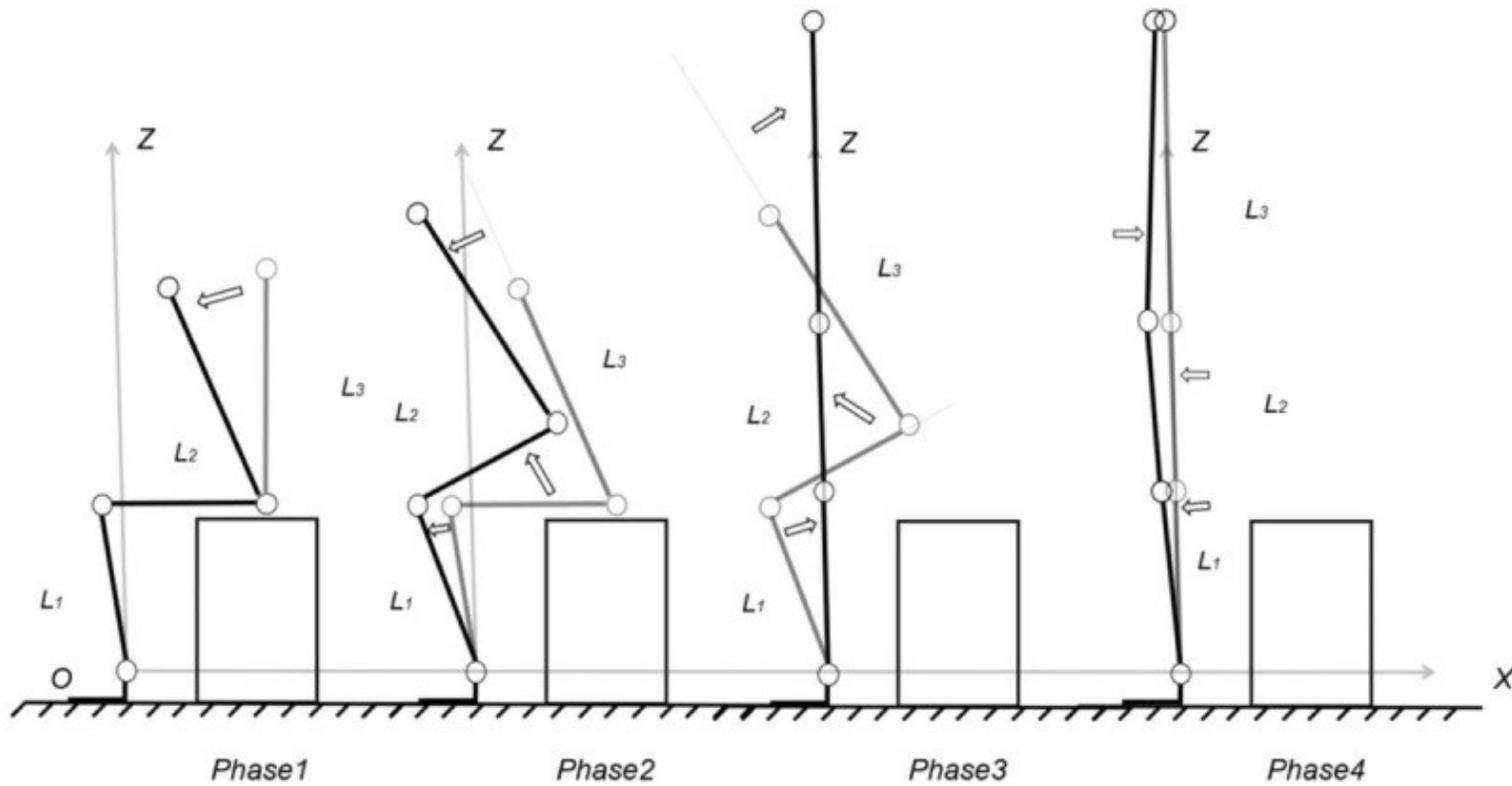


Li J, Xue Q, Yang S, Han X, Zhang S, Li M, Guo J. Kinematic analysis of the human body during sit-to-stand in healthy young adults. *Medicine (Baltimore)*. 2021



Transfer Assist



4) Visual Field Improvement

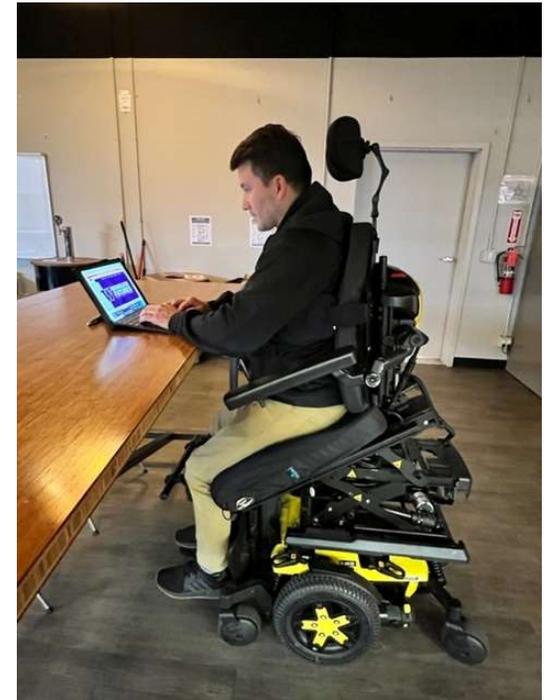

Considerations



Balance and Stability



Trunk Control and Strength



Cognitive Capacity



Bone Density



Body ROM

Potential Candidates for Anterior Tilt

- A client who would benefit from assistance due to impaired trunk control who needs assistance obtaining a higher level of functional reach to complete activities of daily living (ADLs).
- The client can tolerate a more upright body posture the anterior tilt seat function places them into.
- The client can tolerate the partial weight bearing position that the anterior tilt seat function places them into.
- The client has the appropriate range of motion in their lower extremities to tolerate the anterior tilt position

Activity

- Testing Power functions
 - Tilt & recline
 - Tilt, recline & elevating legs
 - Anterior tilt vs. Elevation
- Testing Power functions while driving
 - Rough terrain
 - Navigating slopes

Justification

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

What kind of supports does the NDIS fund?

- Clear goals or aspirations
- Be more independent
- Take part in social activities and work
- Actively take part in the community
- Enjoy an 'Ordinary' Life
- These will need to be related to the client disability



Justification

- Having clear goals relating to disability.
- Is there a clear concern or barrier that needs to be addressed?
 - E.g. Unable to complete recreational activities without fatiguing after 5 minutes.
- Cheaper alternatives have been considered although have not or will not work.
 - E.g. Easy Reacher, manual recline or tilt
- The client has trialled the wheelchair successfully and improved their independence or function whilst completing ADL's.
- Would the provision of the Power Wheelchair save money in the long run?
 - E.g. No need for home modifications, no need to meal deliveries.
- Utilising client feedback



Features of a Power Chair

power:
mobility
The power to move you



QUANTUM[®]
#1 FOR REHAB POWER

Programming Parameters

- Speed
 - Forward
 - Reverse
 - Turning
- Acceleration
- Deceleration
- Joystick Throw
- Tremor Dampening



Memory Seat Positions

Allows for saving of specific positions that incorporate multiple power seat functions, which can be accessed through a programmed button or switch.



Benefits of Memory Seat Positions

Allows for saving of specific positions that incorporate multiple power seat functions, which can be accessed through a programmed button or switch.

- Easily accessed by the user or carers
 - Reduces need to program individual actuators to achieve desired position.
- Programmed functional positions
 - Transfers
 - Drive
 - Rest
 - Bladder Management
 - Pressure Relief
 - Independent repositioning
 - Etc.



TB4 - User Adjustable

User Adjustable:

- Allows the consumer to make changes to the memory positions within that memory slot.
- User Adjustable can be enabled or disabled separately in each memory profile
- Examples could include vehicle access, positions of function for ADL, or positions of comfort for recreation/work activities



Synced Memory Seating Function

The actuators will all move at the same time. The actuators use a timing mechanism that allows all of the actuators to stop at the end position simultaneously



Switches and Shortcut Buttons

Add external switches if hitting buttons/levers is difficult



Using the iAccess Module

- Programmable module that can operate a wide range of functions
- This includes Seating, Bluetooth, Mouse Clicks, Mode Changes, Home Screen Access, and Light Package Control.
- Can be programmed up to 19 functions and have up to 5 pages programmed.



Summary and Take-Aways!

What is important,
most of the time?

Give as much
information as
possible to your
Supplier

Trial both
Indoors &
Outdoors

Establish
Mobility
Device Goals

Work WITH your
client –
Collaborate!

Thank you for your time!

Questions?



PQ-365

DOWNLOAD LINKS



QUANTUM
PRIDE



GET IT ON
Google play

Download on the
App Store

PRIDE
WORLDWIDE
LIVE YOUR BEST!

QUANTUM
#1 SPORTS REHAB POWER!



References

- <https://aci.health.nsw.gov.au/networks/spinal-cord-injury/spinal-seating/module-1>
- Dicianno, B. E., Morgan, A., Lieberman, J., & Rosen, L. (2016). Rehabilitation Engineering & Assistive Technology Society (RESNA) position on the application of wheelchair standing devices: 2013 current state of the literature. *Assistive Technology*, 28(1), 57–62.
- <https://www.resna.org/Portals/0/Documents/Position%20Papers/RESNAWheelchairServiceProvisionGuide.pdf>
- Gauthier, C., Gagnon, D., Jacquemin, G., Duclos, C., Masani, K., & Popovic, M. R. (2012). *Comparison of multidirectional seated postural stability between individuals with spinal cord injury and able-bodied individuals*. *Journal of Rehabilitation Medicine*, 44(9), 820–828
- Pressure Ulcer Prevention and Treatment Following Spinal Cord Injury: A Clinical Practice Guideline for Health-Care Professionals SECOND EDITION S P I N A L C O R D M E D I C I N E. (n.d.-a).
- RESNA Position on the Application of tilt, Recline, and Elevating Legrests for Wheelchairs: 2015 Current state of the Literatures
- RESNA Position of the Application of Seat Elevation Devices for Power Wheelchair Users: Update 2019 Current state of the Literatures
- Schein, R. M., Yang, A., McKernan, G. P., Mesoros, M., Pramana, G., Schmeler, M. R., & Dicianno, B. E. (2021). Effect of the Assistive Technology Professional on the Provision of Mobility Assistive Equipment. *Archives of Physical Medicine and Rehabilitation*, 102(10), 1895–1901. <https://doi.org/10.1016/j.apmr.2021.03.024>

